# Mercaptane

## **SensoriC TBM 2E 50**



### **FEATURES**

Amperometric 2 electrode sensor cell High selectivitiy High reliability Good long term stability

### **TYPICAL APPLICATIONS**

Monitoring of odorants in natural gas applications

#### PART NUMBER INFORMATION

SENSORIC CLASSIC	2441-021-11069
CTL 4 series adaptation	2441-021-14049
CTL 7 series adaptation	2441-021-17079



#### **TECHNICAL SPECIFICATIONS**

Measuring Range 0–50 mg/m<sup>-3</sup>/ 0-14 ppm

Sensitivity Range 3-8 nA/ mg/m<sup>-3</sup>/; 15-40 nA/ mg/m<sup>-3</sup>/ Ethyl-SH (estimated)

Zero Current at  $20^{\circ}$ C  $< \pm 4$  nA < 0.5 mg/m<sup>-3</sup>/ not required Linearity < 5% full scale

Response Time at 20°C

< 40 s calculated from 4 min. exposure time</li>< 90 s calculated from 4 min. exposure time</li>

Long Term Sensitivity Drift < 10% per 10 month

**Operation Conditions** 

Temperature Range -10°C to +40°C

Humidity Range 10–95% r.H., non–condensing


Effect of Humidity no effect

Sensor Life Expectancy > 12 months Warranty 9 months

**Note**: 1 ppm = 3,66 mg/m3




### **OUTPUT vs. TEMPERATURE:**

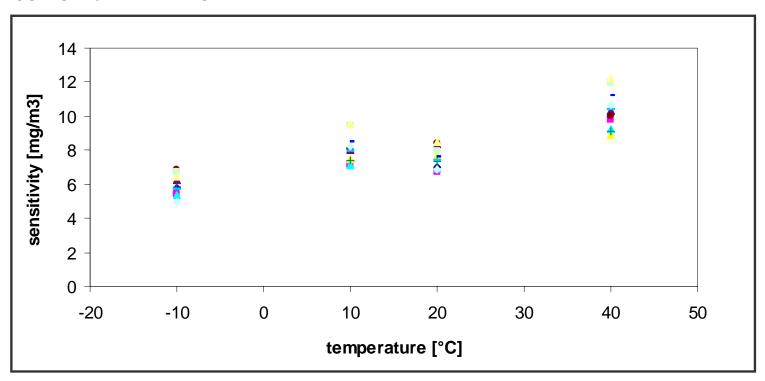



### **ZERO READING vs. TEMPERATURE:**

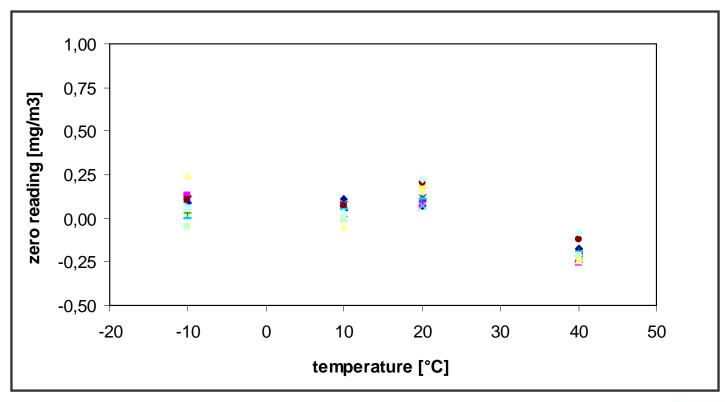



### **CROSS SENSITIVITIES AT 20°C**

Gas	Concentration	Reading [mg/m3]
Alcohols	1000 ppm	0
Carbon Dioxide	1000 ppm	0
Carbon Monoxide	100 ppm	2
Hydrocarbons	% range	0
Hydrogen	1 %	0
Hydrogen Sulfide	20 ppm	01
Isopropanol	200 ppm	0
Methane	100 %	0
Nitrogen	100 %	0
Nitrogen Dioxide	10 ppm	-80
Sulfur Dioxide	20 ppm	0

<sup>1)</sup> With inboard filter; to remove TLV levels of interfering gases; continuous high level exposure may reduce the efficiency of the filter material.

#### Notes:

- 1. Interference factors may differ from sensor to sensor and with life time. It is not adviseable to calibrate with interference gases.
- 2. This table does not claim to be complete. The sensor might also be sensitive to other gases.

